

# SENSOR OF ROTATIONAL MOVEMENT AROUND VERTICAL AXIS FOR SEISMIC MEASUREMENT

Jaroslav Strunc<sup>1</sup>, Stanislav Dado<sup>2</sup>, Jiri Buben<sup>3</sup>

<sup>1</sup> Institute of Rock Structure and Mechanics AS CR, Prague, Czech Republic, strunc@irms.cas.cz

<sup>2</sup> Faculty of Electrical Engineering, Czech Technical University, Prague, Czech Republic, dado@fel.cvut.cz

<sup>3</sup> Institute of Rock Structure and Mechanics AS CR, Prague, Czech Republic, buben@irms.cas.cz

**Abstract:** Studying of rotational components of ground movements belong among emerging approaches in recent geophysics. Rotations can be observed using the dense seismic arrays (micro-arrays, small aperture arrays) formed from classic three-dimensional seismic sensors. The aim of this project is a construction of portable, high-definition sensor of rotational movement around vertical axis. This sensor is based on measuring of changes of capacitance of differential capacitor.

**Keywords:** rotation, seismic, capacitance

## 1. INTRODUCTION

The rotation components of seismic ground motion can be radiated from the source or can be generated when seismic waves spread through anisotropic (micromorphic) rock massif or rise as the response of building structures on dilatational excitation. The rotation component of strong ground motion can represent a non-negligible contribution to the whole earthquake hazard to building structures in near zones. The excitation of rotation vibration depends on the structure of subsoil, on the dynamic response of building structures and on build-in components. This holds especially for building constructions with prevailing linear shape, such as pipelines and rapid rail lines and for objects with great seismic risk (e.g. nuclear power plants), great seismic vulnerability and for historical buildings.


Actually there is no mobile seismic sensor of such kind of motion. Rotational movements are evaluated from signals of classic three-dimensional seismic sensors in dense-arrays [1]. There is only one permanent station for measuring rotational movements – in Germany. It is based on laser interferometer [2].

## 2. METHODS

The angular deflections of a rotation seismometer have very small amplitudes (from nanoradians to microradians) at long periods of teleseismic events. Therefore the deflection-to-voltage transducer must be extremely sensitive especially for long periods of motion.


Our sensor of this kind of movement is realized as a differential capacitor in shape of one twelfth of roundel (fig. 1). It is mounted on a long arm fixed by balancer in stabilized position. The balance wheel hangs on a straight spring realizing the sensor of rotation around the vertical axis. Its natural oscillations are damped electro-magnetically using strong permanent magnets and cooper lamellas at the opposite side of the arm. The first idea was to build as large

capacitor as one third (120 degree arc) of disc is but we hit the limit of the manufacturing technology. Maximal size of board in required accuracy ( $10^{-1}$  mm) is 500 mm × 250 mm.

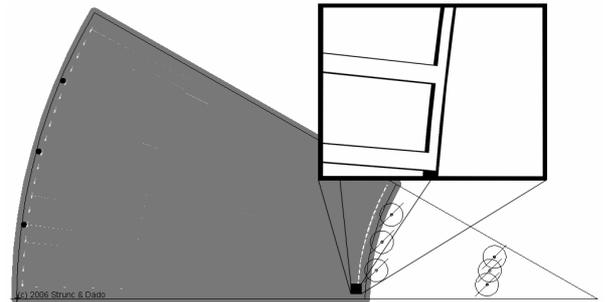

**Fig. 1 Board with zoomed electrodes**

Active parts of capacitor are three desks (fig. 1) with electrodes made by technology of printed board circuits (PCB). Two desks are fixed as stators and one is moveable around vertical axis (rotor). Differential capacity is not depending on the distance between the inner and outer board. Therefore it is possible to leave out the vertical movements. Electrodes are designed as sectors (radial rays) with half horizontal covering (fig. 2).

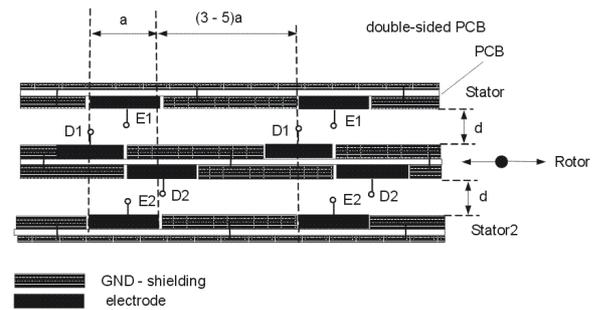

**Fig. 2 Side view of boards with electrodes**

Capacitance between each static desk and the rotational one increases or decreases depending on the sense of the rotation. These changes in order of femto-Farads (fF), are monitored by a sensitive capacity bridge.

The area of whole capacitor can be calculated by (1).

$$S_{el} = N \cdot \varphi_{el} \cdot (r_{out}^2 - r_{in}^2) \quad (1)$$

Where  $N$  is number of rays,  $\varphi_{el}$  is angle of electrode arc,  $r_{out}$  and  $r_{in}$  are outer and inner radius.

Final capacitance of the sensor is (2).

$$C = \varepsilon_0 \cdot \varepsilon_r \cdot \frac{N}{d} \cdot \varphi_{el} \cdot (r_{out}^2 - r_{in}^2) \quad (2)$$

Where  $d$  is desk spacing,  $\varepsilon_0$  and  $\varepsilon_r$  are the permittivity of vacuum and the relative permittivity of air. Differential capacitor does not depend on the position of the middle electrode when the outlying ones are static.


### 3. IMPLEMENTATION

As mentioned above this sensor is realized by the printed board circuit technology. We were handicapped in dimensions because of only a few manufacturers make boards larger than obvious ones for job-order electronics.

In expectation of future changes we had made easy adjustable scripts for program Eagle and for preparing data in Gerber format for manufacturing.

The final shape of our sensor is created as 30 degrees arc-board with external radius 500 mm and internal radius 200 mm (fig. 1). Active part is from 19 electrodes on each side (layer) of the central desk. Electrodes are realized as 5 mrad segments and are 290 mm long. Phase shift of these layers is 5 mrad. Layer diagrams are shown as zoomed detail. Active chart is surrounded by large grounded area. Central desk is moveable around centre of rotation. At distance of 1 mm from both sides will be mounted stationary boards with opposite phase-shifted shape – shift is 2.5 mrad at the initial state, zero balance (fig. 2).

There is linear relation between capacitance and deflection angle (fig. 3). In this figure you can see dependence on increasing of the coverage. For example the deflection  $10^{-5}$  rad causes change capacitance in order of 170 fF ( $1.7e10^{-13}$  F).

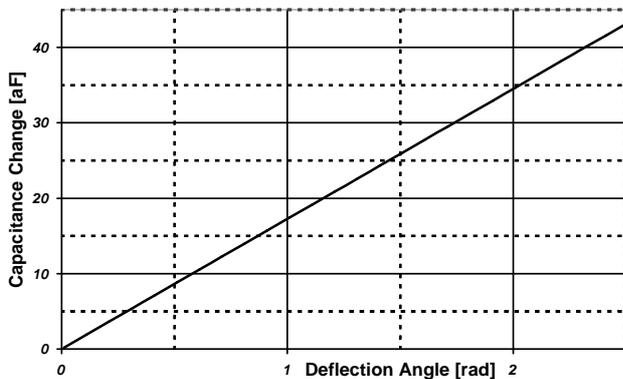


**Fig. 3 Linear relation of deflection and capacitance**

This change is detectable by high precision balancing bridge. At fig. 4 is a principle diagram of measuring the capacitance [3]. There are used two capacitors – measuring  $C_m$ , and reference  $C_{ref}$ . Two sources of alternating currents  $U_m$  and  $U_{reg}$  with opposite phases are used. The operation amplifier serves as a current-to-voltage converter. The output signal  $U_{reg}$  regulates the amplitude of the source  $U_m$ . In the equilibrium state ( $I_0 = 0$ ) it holds the relation (3).

$$\frac{C_m}{C_{ref}} = \frac{U_m(j\omega)}{U_{ref}(j\omega)} \Big|_{I_0(j\omega)=0} \quad (3)$$

The output is registered by a high definition, 21-bit, A/D converter Tedia into personal computer. In the future we suppose developing of a microcontroller-based device for operation in-situ.

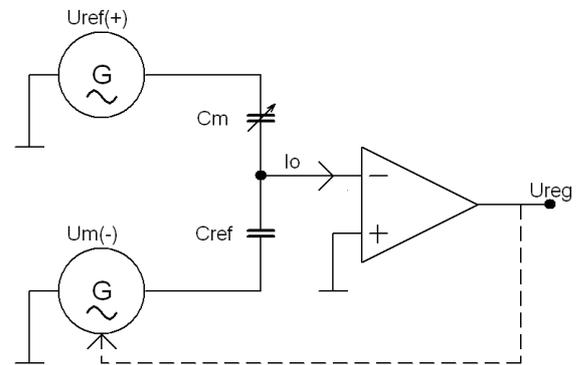

**Fig. 4 Measuring small capacitances**

### 4. RESULTS

The first aim is reliable measuring of strong rotations induced at quarry blasts and near epicenters of earthquakes. Vibrations, excited by explosions can be used for investigation of amplitude attenuation relations of strong ground vibration. The parameters of anisotropic attenuation relations are important namely for seismic micro zoning of the storage sites of wastes. The second aim is measuring of weak long-period teleseismic waves. The first one seems to be satisfied regarding supposed amplitudes in this case in order of  $10^{-3}$  rad. After some successful field trials we will modify sensor to reach more sensitivity. For this operation can be used one-chip microcomputer providing real-time filtering and coherent demodulation.

### REFERENCES

- [1] B. S. Huang, Ground rotational motions of the 1999 Chi-Chi, Taiwan earthquake as inferred from dense array observations, Geophysical Research Letters, Vol. 30, No. 6, 2003
- [2] W. Suryanto, J. Wassermann, H. Igel, A. Cochard, D. Vollmer, F. Scherbaum, A. Velikoseltsev, U. Schreiber, First comparison of seismic array derived rotations with direct ring laser measurements of rotational ground motion, Bull. Seismo. Soc. Amer., 2006, in publication
- [3] S. Dado, M. Kreidl, Senzory a merici obvodu (Sensors and Measuring Circuits), CVUT, 1999, Prague
- [4] J. Vejdecký, S. Dado, Merení permitivity plynu (Measurement of Permittivity of Gases), Workshop, 2003, Prague
- [5] V. Rudajev, J. Buben, M. Broz, J. Strunc and L. Zanda, Recording Rotation Component of Strong Ground Motion, Springer-Verlag, 2005, not published

### ACKNOWLEDGEMENT

This work is supported by IRSM AS CR as a part of the Institute Research Plan number A VOZ30460519.